

In re: Gross et al.  
Serial No.: 10/686,762  
Filed: October 16, 2003  
Page 8 of 18

### REMARKS

Claims 1-29 are pending. Claims 6-9, 14-17, 23, 24 and 29 stand rejected under 35 U.S.C. §112, second paragraph, as being indefinite. Claims 1-3, 8-12, 16-21 and 24-29 stand rejected under 35 U.S.C. §102(b) as being anticipated by U.S. Patent No. 6,032,612 to Williams ("Williams"). Claims 5-7, 13-15, 22, 23, 26, 27 and 29 stand rejected under 35 U.S.C. §103(a) as being unpatentable over Williams. Claims 4, 21 and 28 stand rejected under 35 U.S.C. §103(a) as being unpatentable over Williams in view of U.S. Patent No. 4,040,388 to Miller ("Miller").

Applicants have amended Claims 6-9, 14-17, 23, 24 and 29 to overcome the rejection under 35 U.S.C. §112, second paragraph. Applicants have also amended Claims 1, 2, 11, 19, 26 and 27 to clarify Applicants' invention. Applicants respectfully traverse the rejections under 35 U.S.C. §102 and 35 U.S.C. §103 for at least the reasons set forth below.

**BEST AVAILABLE COPY**

In re: Gross et al.  
 Serial No.: 10/686,762  
 Filed: October 16, 2003  
 Page 9 of 18



### §112 Rejections Are Overcome

Applicants have amended Claims 6-9, 14-17, 23, 24 and 29 as indicated above pursuant to the Examiner's suggestions. Accordingly, the indefinite rejection under 35 U.S.C. §112, second paragraph, is overcome.

### §102 Rejections Are Overcome

A claim is anticipated under 35 U.S.C. §102 if each claimed element is found in a single prior art reference. *Scripps Clinic & Research Foundation v. Genentech, Inc.*, 927 F.2d 1565, 1576 (Fed. Cir. 1991); *Carella v. Starlight Archery and Pro Line Co.*, 804 F.2d 135, 138 (Fed. Cir. 1986). There must be no difference between the claimed invention and the reference disclosure, as viewed by an ordinary artisan. *Scripps Clinic & Research Foundation v. Genentech, Inc.*, 927 F.2d at 1576.

The Action has taken the position that the egg engaging member 26 of the bottom injection device 25' illustrated in Fig. 10 of Williams is an egg support assembly. Figs. 3 and 10 from Williams are set forth below.

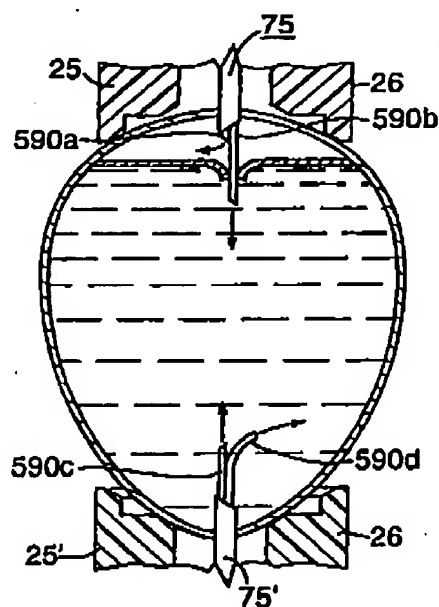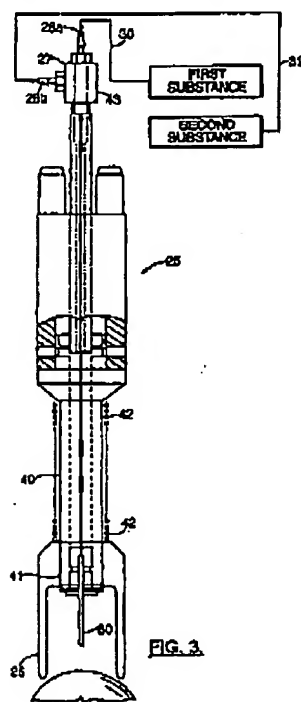

**FIG. 10.**

In re: Gross et al.  
Serial No.: 10/686,762  
Filed: October 16, 2003  
Page 10 of 18

The bottom injection device 25' illustrated in Fig. 10 of Williams is identical in structure and function to the top injection device 25, with the exception that the illustrated bottom injection device 25' includes two needles for injecting material into an egg. Williams specifically states that "the description describes a unit with a single multi-site injection device 25 (shown as a top injection device) but the description also applies to an apparatus with multiple injection devices 25', 25" (exemplarily [sic] shown in Figs. 10 and 11), or alternatively, one or more of single bottom or side devices." (Williams, Col. 6, Lines 16-21). In describing the injection device 25, Williams states:

The device includes an egg locating member, or *egg engaging member 26*, connected to the body member bottom end portion, which as illustrated *is slidably connected to the body member and includes a spring 42 to both cushion the engagement*, and hold the egg in place during the downstroke of the injection head. (Williams, Col. 7, Lines 3-8; emphasis added).

The Action is confusing an injection device 25' that is configured to inject an egg from the bottom of the egg with a support pedestal of the present invention. The egg engaging member 26 does not serve the function of a support that is configured to support an egg against the opposing force of an injection device. Nothing in Williams teaches or suggests supporting an egg against the opposing force of injection device 25 with the injection device 25'. Fig. 10 of Williams is merely provided to show that multiple injection devices may be utilized and/or that an injection device may be utilized at different locations relative to an egg. As viewed by the ordinary artisan, there is a great difference between a support pedestal of the present invention and the injection device 25' of Williams.

Moreover, Applicants respectfully assert that the injection device 25' of Williams teaches away from supporting an egg during injection. The egg engaging member 26 of the injection device 25' is slidably connected to the body member of the injection device 25'. Such a configuration cannot support an egg against downward forces caused during injection by an injection device located on top of an egg.

Notwithstanding the above, Applicants have amended independent Claim 1 to recite an *in ovo* injection apparatus, comprising:

an egg support assembly positioned beneath the carrier that is configured to *solidly* support each egg in the carrier during contact therewith by a respective

In re: Gross et al.  
Serial No.: 10/686,762  
Filed: October 16, 2003  
Page 11 of 18

*injection device and to prevent each egg from being pushed downwardly into the carrier by a respective injection device.*

Independent Claims 11, 19 and 26 have been similarly amended.

Williams fails to teach or suggest supporting an egg from being pushed downwardly into a carrier by an injection device. Moreover, the injection device described in Williams is unsuitable for solidly supporting an egg and preventing an egg from being pushed downwardly into a carrier by an injection device as suggested by the Action. Applicants respectfully submit that, because Williams does not disclose all of the recited elements of independent Claims 1, 11, 19 and 26, these claims and all claims depending therefrom are not anticipated by Williams.

Applicants' amended Claim 2 recites an egg support assembly that comprises:  
a frame movable between an operative position and a retracted position;  
a plate attached to the frame and comprising an array of openings formed therein; and  
a plurality of pedestals, each pedestal removably and snugly secured within a respective one of the openings, wherein each pedestal comprises a free end portion configured to engage an egg within the carrier when the frame is in the operative position.

The recited structure of Claim 2 is illustrated in Figs. 7 and 8 from Applicants' application, which are set forth below.


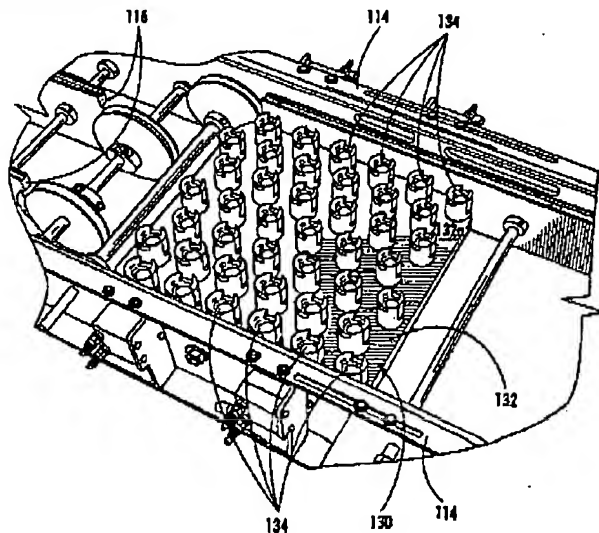


FIG. 7

In re: Gross et al.  
 Serial No.: 10/686,762  
 Filed: October 16, 2003  
 Page 12 of 18

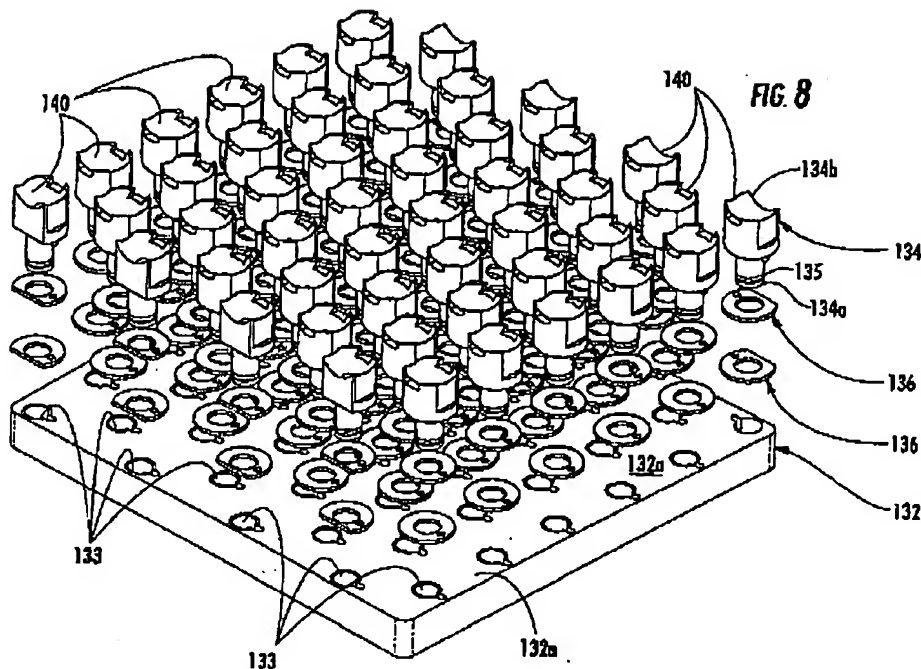


Applicants' egg support assembly 130 is configured to support each egg in an egg flat during contact by an egg injection device 25. The illustrated egg support assembly 130 includes a plate 132 having a plurality of pedestals 134 extending from an upper surface 132a of the plate 132. Each pedestal 134 is configured to support a respective egg in an egg flat positioned thereover. The plate 132 includes an array of openings 133 formed therein in a pattern matching the array of pockets in an egg flat. Each pedestal 134 is removably secured within a respective one of the plate openings 133. Each pedestal 134 includes a proximal end 134a and a distal free end 134b. An O-ring 135 is secured to each pedestal adjacent the proximal end 134a and provides a *snug, friction fit* when the proximal end 134a is disposed within a respective opening 133. One or more shims 136 may be utilized to adjust the height of the distal end 134b of each pedestal 134 above the plate surface 132a, as illustrated. The pedestals 134 are configured to be easily removed from the plate 132 such that shims can be added and removed as necessary.

The Action concedes that Williams fails to explicitly state the construction of the lower egg support assembly. (Action, Page 3). However, the Action concludes that "it would be

In re: Gross et al.  
 Serial No.: 10/686,762  
 Filed: October 16, 2003  
 Page 13 of 18

fair to take the disclosed structure of the upper assembly as a guide for the lower assembly." (Action, Page 3). The Action has taken the position that the structure of the injection apparatus of Fig. 2 of Williams anticipates the recited structure of the egg support assembly in Applicants' Claim 2.

Fig. 2 from Williams is set forth below:

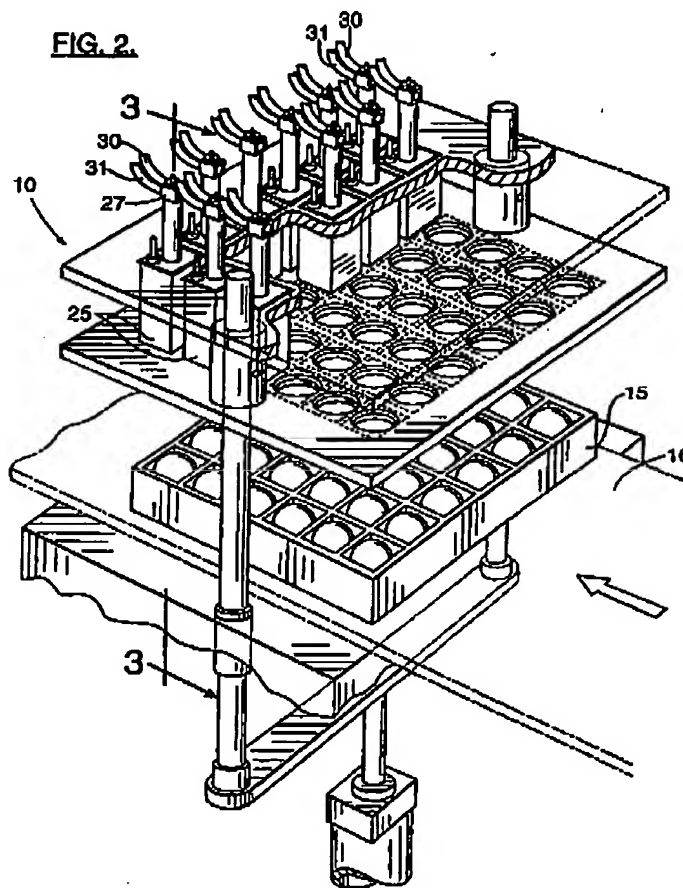

The illustrated Williams apparatus 10 is an embodiment of the Embrex® Inovoject® Egg Injection System manufactured and sold by the assignee of the present invention and application. The apparatus 10 includes a flat 15, a stationary base 16, and a plurality of injection delivery devices 25 with fluid delivery means such as lumens or needle(s) 90 positioned therein. The flat 15 holds a plurality of eggs 20 in a substantially






In re: Gross et al.  
Serial No.: 10/686,762  
Filed: October 16, 2003  
Page 14 of 18

upright and aligned position. The flat 15 is configured to provide external access to predetermined areas of the eggs 20. The egg is held in by the flat 15 so that a respective one egg is in proper alignment relative to a corresponding one of the injection devices 25 as the injection device 25 advances towards the base 16 of the apparatus. Each of the injection devices 25 has opposing first and second ends 26, 27. Each injection device 25 has a first extended position and a second retracted position. Upon extension of the injection device 25, the first end 26 is configured to contact and rest against predetermined areas of the external egg shell. When not injecting, the injection devices 25 are retracted to rest a predetermined distance above the eggs and stationary base 16.

The Williams apparatus 10 includes a generally horizontally oriented tooling plate with openings therethrough. An injection device 25 rests generally vertically in each respective opening in the tooling plate. When the tooling plate is lowered and the egg engaging member 26 of each resting injection device 25 strikes an egg to be injected, the injection device 25 stops while the tooling plate proceeds downwardly until the injection device 25 disengages from the tooling plate. At this point, the injection device 25 is free to move in a translational direction independent of the tooling plate to seek and come to rest upon the top most portion of an egg, even if that egg is slightly tilted. When the tooling plate is raised, it reengages the injection device 25, straightens the injection device 25 with respect to the vertical, and carries it upwardly and away from the egg being injected.

The injection devices 25 are slidably disposed within the openings in the tooling plate and can move independent of the tooling plate. This is in sharp contrast with Applicants' egg support assembly 130 wherein each pedestal 134 is disposed snugly within a respective opening 133 in the plate 132 and wherein movement of the pedestals 134 is *not* independent of the plate 132. As illustrated in Figs. 15A-15E of Applicants' application, and set forth below, each pedestal 134 is in the same contacting relationship with the plate 132, no matter what the position of the plate 132 is.

In re: Gross et al.  
 Serial No.: 10/686,762  
 Filed: October 16, 2003  
 Page 15 of 18

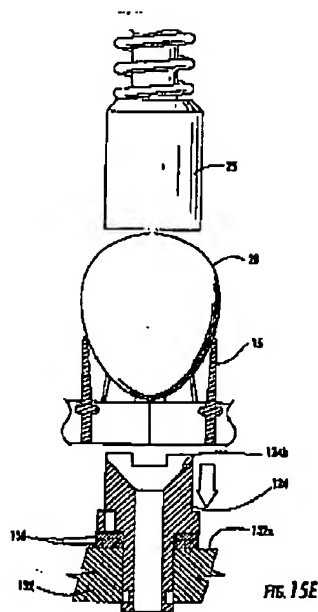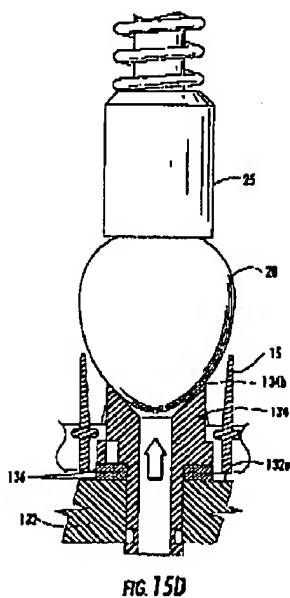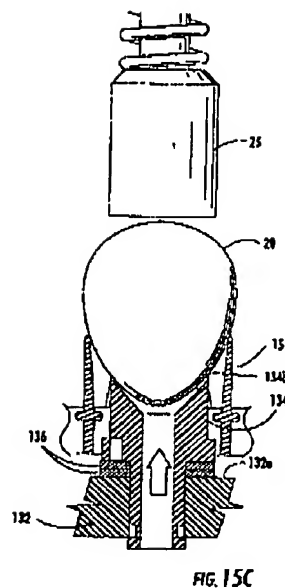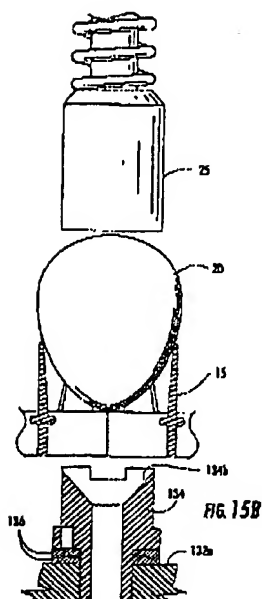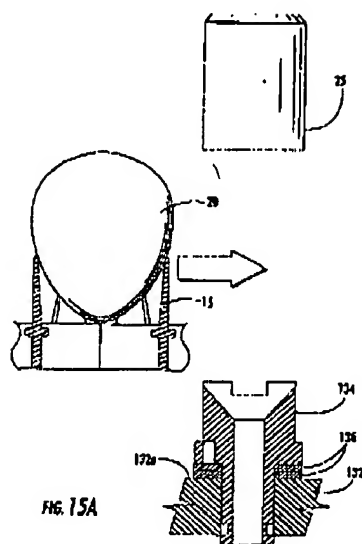



In re: Gross et al.  
Serial No.: 10/686,762  
Filed: October 16, 2003  
Page 16 of 18

Notwithstanding the above, Applicants have amended Claim 2 to recite that each pedestal is removably *and snugly* secured within a respective one of the openings in the plate. Claims 11, 19 and 27 have been similarly amended. Accordingly, Applicants respectfully submit that, because Williams does not disclose all of the recited elements of Claim 2, this claim is not anticipated by Williams. Similarly, Claims 11, 19 and 27 are not anticipated by Williams.

With respect to Claim 3, the Action states, and without citation, that Williams further discloses "wherein the egg support assembly is operatively associated with the plurality of injection devices 25 such that each pedestal moves upwardly through a respective opening in the carrier 15 to support an egg 20 as a respective injection device 25 makes contact with the egg 20." Applicants respectfully assert that Williams does not disclose any such thing, and respectfully request that the passage within Williams that discloses this be identified. Again, the Action is confusing an injection device 25' that is configured to inject an egg from the bottom of the egg with a support pedestal of the present invention. Accordingly, Claim 3 is not anticipated by Williams. For at least the same reasons, Claims 12 and 20 are not anticipated by Williams.

In view of the above, the rejections under 35 U.S.C. §102 are overcome.

### **§103 Rejections Are Overcome**

A determination under §103 that an invention would have been obvious to someone of ordinary skill in the art is a conclusion of law based on fact. *Panduit Corp. v. Dennison Mfg. Co.* 810 F.2d 1593, 1 U.S.P.Q.2d 1593 (Fed. Cir. 1987), *cert. denied*, 107 S.Ct. 2187. After the involved facts are determined, the decision maker must then make the legal determination of whether the claimed invention as a whole would have been obvious to a person having ordinary skill in the art at the time the invention was unknown, and just before it was made. *Id.* at 1596. The United States Patent and Trademark Office (USPTO) has the initial burden under § 103 to establish a *prima facie* case of obviousness. *In re Fine*, 837 F.2d 1071, 5 U.S.P.Q.2d 1596, 1598 (Fed. Cir. 1988).

To establish a *prima facie* case of obviousness, the prior art reference or references when combined must teach or suggest *all* the recitations of the claims, and there must be some suggestion or motivation, either in the references themselves or in the

In re: Gross et al.  
Serial No.: 10/686,762  
Filed: October 16, 2003  
Page 17 of 18

knowledge generally available to one of ordinary skill in the art, to modify the reference or to combine reference teachings. M.P.E.P. § 2143. The mere fact that references can be combined or modified does not render the resultant combination obvious unless the prior art also suggests the desirability of the combination. M.P.E.P. § 2143.01(citing *In re Mills*, 916 F.2d 680, 16 U.S.P.Q.2d 1430 (Fed. Cir. 1990)). As emphasized by the Court of Appeals for the Federal Circuit, to support combining references, evidence of a suggestion, teaching, or motivation to combine must be **clear and particular**, and this requirement for clear and particular evidence is not met by broad and conclusory statements about the teachings of references. *In re Dembiczak*, 50 U.S.P.Q.2d 1614, 1617 (Fed. Cir. 1999). In an even more recent decision, the Court of Appeals for the Federal Circuit has stated that, to support combining or modifying references, there must be **particular** evidence from the prior art as to the reason the skilled artisan, with no knowledge of the claimed invention, would have selected these components for combination in the manner claimed. *In re Kotzab*, 55 U.S.P.Q.2d 1313, 1317 (Fed. Cir. 2000).

Furthermore, as recently stated by the Federal Circuit with regard to the selection and combination of references:

This factual question of motivation is material to patentability, and could not be resolved on subjective belief and unknown authority. It is improper, in determining whether a person of ordinary skill would have been led to this combination of references, simply to "[use] that which the inventor taught against its teacher." W.L. Gore v. Garlock, Inc., 721 F.2d 1540, 1553, 220 USPQ 303, 312-13 (Fed. Cir. 1983). Thus the Board must not only assure that the requisite findings are made, based on evidence of record, but must also explain the reasoning by which the findings are deemed to support the agency's conclusion....

*In re Sang Su Lee*, 277 F.3d 1338, 1343 (Fed. Cir. 2002).


For at least the same reasons set forth above with respect to 35 U.S.C. §102, Applicants respectfully assert that the primary reference, Williams, fails to teach or suggest the recitations of Applicants' independent claims, particularly as amended above, and all claims depending therefrom. Specifically, Williams fails to teach or suggest an *in ovo* injection apparatus, comprising an egg support assembly positioned beneath an egg carrier that is configured to **solidly** support each egg in the carrier during contact therewith by a respective injection device **and to prevent each egg from being pushed downwardly into the carrier by**

In re: Gross et al.  
Serial No.: 10/686,762  
Filed: October 16, 2003  
Page 18 of 18

*a respective injection device* as recited in each of Applicants' amended independent claims (Claims 1, 11, 19 and 26). As discussed above, the Action is confusing an injection device 25' that is configured to inject an egg from the bottom of the egg with a support pedestal of the present invention. Accordingly, Applicants respectfully request withdrawal of the present rejections under 35 U.S.C. §103.

In view of the above, it is respectfully submitted that this application is in condition for allowance, which action is respectfully requested.

Respectfully submitted,




Needham J. Boddie, II  
Attorney for Applicants  
Registration No. 40,519

USPTO Customer No. 20792  
Myers Bigel Sibley & Sajovec, P.A.  
Post Office Box 37428  
Raleigh, North Carolina 27627  
Telephone: (919) 854-1400  
Facsimile: (919) 854-1401

**CERTIFICATION OF FACSIMILE TRANSMISSION UNDER 37 CFR § 1.8**

I hereby certify that this correspondence is being transmitted by facsimile to the U.S. Patent and Trademark Office Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450 on September 16, 2004 via facsimile number 703-872-9306.

  
Erin A. Campion

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

**BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ **BLACK BORDERS**
- ☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- ☐ **FADED TEXT OR DRAWING**
- ☐ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- ☐ **SKEWED/SLANTED IMAGES**
- ☐ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- ☐ **GRAY SCALE DOCUMENTS**
- ☐ **LINES OR MARKS ON ORIGINAL DOCUMENT**
- ☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**
- ☐ **OTHER:** \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**